

Calibration Report: Pyranometer CM22-040100

Fred M. Denn and Bryan E. Fabbri.
Science Systems & Applications, Inc., Hampton, Virginia.
Document date 2020 October 30.

Calibration date: 2020-10-15.
Next calibration: 2022-10-15.
Reference standard: AHF-31041

The calibration coefficients and their associated uncertainties (U95%) have been determined for one pyrheliometer. The unit of the calibration coefficient (S) is $\mu\text{V}/(\text{W}/\text{m}^2)$. The reference standard was Eppley Laboratories Inc., absolute cavity radiometer AHF31041, with its associated data acquisition system. Cavity AHF31041 participated in the 2015 International Pyrheliometer Comparison (IPC XII) at the Physikalisch-Meteorologisches Observatorium, in Davos Switzerland. It is therefore traceable to the World Radiation Reference. Cavity AHF31041's calibration is verified annually at the National Pyrheliometer Comparison held at the National Renewable Energy Laboratory in Golden Colorado, most recently in September of 2019.

The sensitivity factors and their associated uncertainties (95%) are as follows:

Sensor	S ($\mu\text{V}/(\text{W}/\text{m}^2) \pm \text{U95\%}$)	Method
CM22-040100	9.108 \pm 0.89%	relative to CM31-000507 and CM22-000025

Application


$$I = (\mu\text{V output})/S \pm \text{sqrt}(2)*\text{U95\%}$$

Where: I = the irradiance measured by the pyranometer
($\mu\text{V output}$) = microvolt output of the pyranometer
S = calibration coefficient of the pyranometer
U95% = the 95 % confidence level

Some supporting plots, a list of past calibration values, and a brief description of the calibration process is presented below.

Pyranometer Calibration Plot


- /Users/fred.denn/Forsun/SRB/Calibrations/Cavity_second_based/Cal_relative_cav_groups/group_case_cm22_040100_RelativeTo_cm22_000025_2020-10-06.l
- /Users/fred.denn/Forsun/SRB/Calibrations/Cavity_second_based/Cal_relative_cav_groups/group_case_cm22_040100_RelativeTo_cm22_000025_2020-10-07.l
- ◇ /Users/fred.denn/Forsun/SRB/Calibrations/Cavity_second_based/Cal_relative_cav_groups/group_case_cm22_040100_RelativeTo_cm22_000025_2020-10-08.l

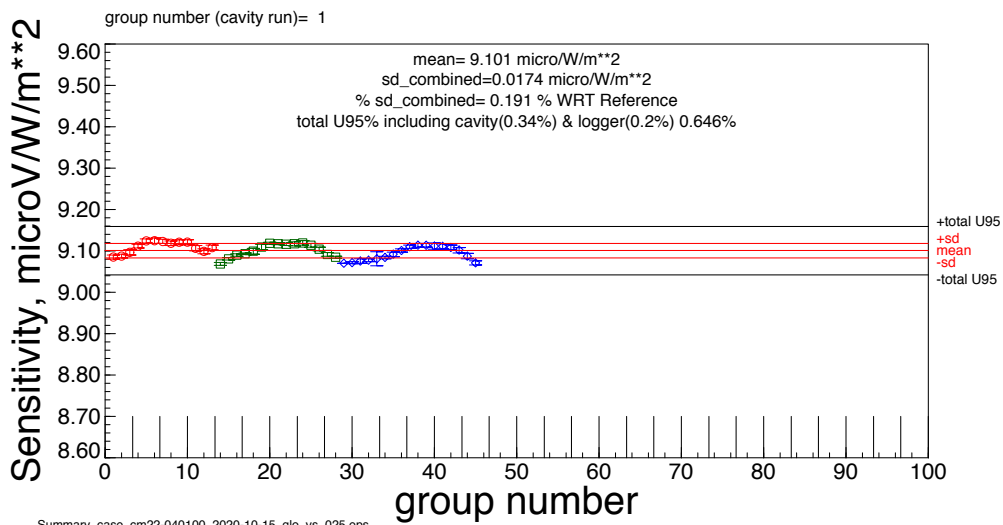


Summary case cm22-040100_2020-10-15_glo_vs_025.eps
Oct 29 10:27:16 2020
/Users/fred.denn/Forsun/SRB/Calibrations/Cavity_second_based/Cal_pyr_groups

Pyranometer Calibration Plot

○ /Users/fred.denn/Forsun/SRB/Calibrations/Cavity_second_based/Cal_relative_cav_groups/group_case_cm22_040100_RelativeTo_cm31_000507_2020-10-06.l
□ /Users/fred.denn/Forsun/SRB/Calibrations/Cavity_second_based/Cal_relative_cav_groups/group_case_cm22_040100_RelativeTo_cm31_000507_2020-10-07.l
◇ /Users/fred.denn/Forsun/SRB/Calibrations/Cavity_second_based/Cal_relative_cav_groups/group_case_cm22_040100_RelativeTo_cm31_000507_2020-10-08.l

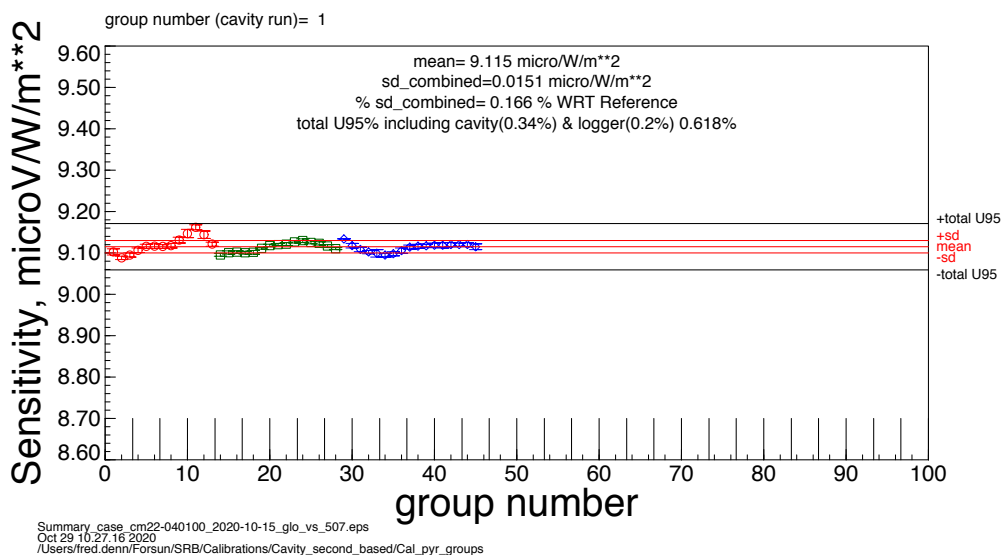

Relative calibration coefficients for several days. Each symbol represents a cavity run which is approximately 25 minutes. These data are combined to get a final calibration coefficient for the entire, multi-day, calibration session. The top plot is CM22-040100 relative to CM22-000025, the bottom plot is CM22-040100 relative to CM31-000507. The final calibration value is the mean of the two cases and the final uncertainty is root mean square of the two uncertainties.

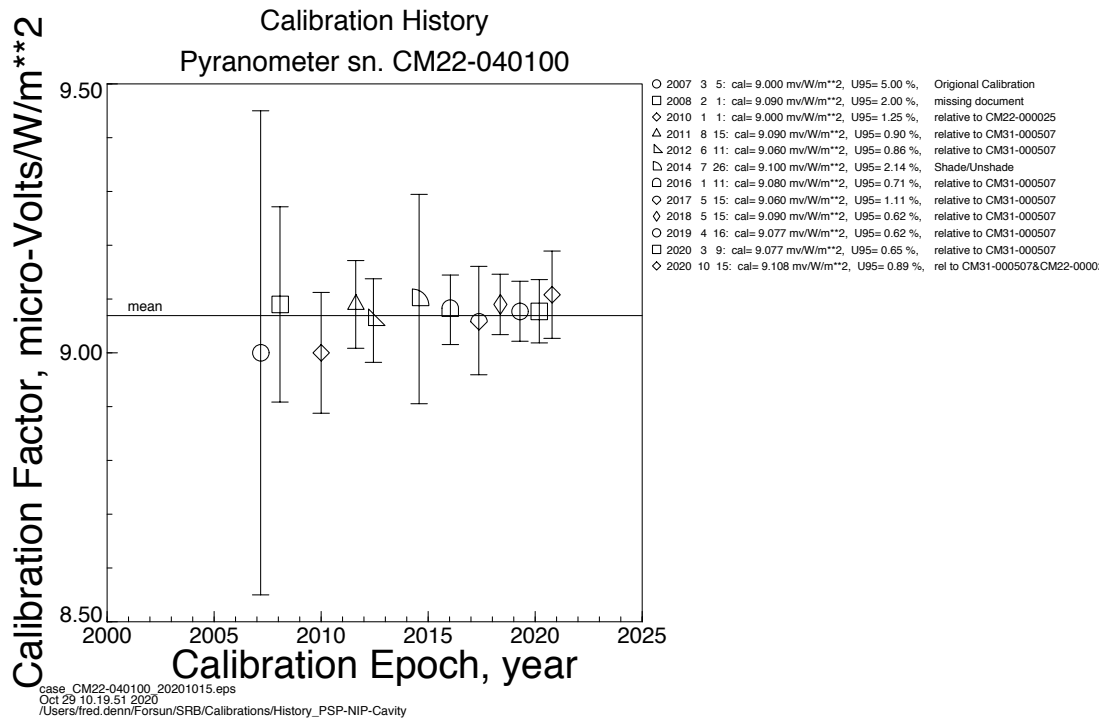

Calibration history for pyranometer CM22-040100. The solid horizontal line represents the mean value. The symbols and their error bars represent the mean and U95 of each calibration event. The column on the right presents numerical values for each calibration event and a brief description of the calibration method used.

CALIBRATION HISTORIES

(doy = day of year)

Pyranometer: Kipp and Zonen CM22-040100

date	doy	S ($\mu\text{V}/\text{W}/\text{m}^2$)	U95 (%)	calibration type
2020-10-15	---	9.108	0.89	relative to CM31-000507
2020-03-09	69	9.077	0.65	relative to CM31-000507
2019-04-16	106	9.077	0.62	relative to CM31-000507
2018-05-15	135	9.09	0.62	relative to CM31-000507
2017-05-02	122	9.06	1.11	relative to CM31-000507
2016-01-11	011	9.08	0.71	relative to CM31-000507
2014-07-26	206	9.10	2.14 (%)	shade/unshade
2012-06-11	163	9.06	0.86 (%)	relative to CM31-000507
2011-08-25	237	9.09	1.316	Forgan's alternate
2010-01-01	001	9.00	1.316	Forgan's alternate
2008-02-02	033	9.09	1.316	Forgan's alternate
2007-03-05	064	9.00	5.00	manufacturers original

A Very Brief Description of the Calibration Process.

- 1) Deploy the Cavity Radiometer, select the 4 second data collection parameter file. Start the cavity calibration process.
- 2) Modify the field radiometer program, set the parameter that causes one second data collection.
- 3) Prepare the tracker hardware to operate in manual shade/unshade mode. Either in manual mode or with the automatic pneumatic cylinder.
- 4) Start the cavity in sun-run mode, do this on a minute that is a multiple of 5 into the hour. Note a cavity calibration and sun-run takes almost 30 minutes.
- 5) Raise or lower the tracker shading balls every 5 minutes, on multiples of 5 minutes into the hour.
- 6) Continue this process as long as sky conditions permit while cavity irradiance is greater than 700 Watts/meter**2.
- 7) On both the cavity computer and the field radiometer computer, open a web browser and email the data files to the data processing computer, Files could also be copied to an external memory stick.
- 8) Remove data that is flagged as “unstable” in the cavity data file.
- 9) Run a splitter program on the field radiometer file to generate a separate file for the shaded and unshaded periods for each instrument.
- 10) Run a plotting program on each data file so the data can be reviewed for: cloud events; bad shading; errors in the splitting routine; etc. Remove bad data.
- 11) Run a calibration program to determine the calibration coefficient for each instrument.
- 12) Combine several days of calibration data to get a final calibration coefficient.
- 13) Produce a calibration document, such as this one, for each instrument. To be considered valid a calibration must be both traceable to recognized standards, in this case the World Radiation Reference (WRR) in Davos Switzerland, and documented.