

# Calibration Report: Pyrheliometer

## Kipp and Zonen CH1-960133

World Meteorological Organization number 39017  
(For the Baseline Radiation Network)

Fred M. Denn and Bryan E. Fabbri.  
Science Systems & Applications, Inc., Hampton, Virginia

Document date, 2026 May 30

Calibration date: 2026 May 30.

Next calibration due: 2028 May 30.

Reference standard: AHF-31041, minimum irradiance 700 W/m\*\*2.

The calibration coefficients and their associated uncertainties (U95%) have been determined for one pyrheliometer. The unit of the calibration coefficient (S) is  $\mu\text{V}/(\text{W}/\text{m}^2)$ . The reference standard was Eppley Laboratories Inc., absolute cavity radiometer AHF-31041, with its associated data acquisition system. The AHF-31041 calibration is traceable Through the Golden Colorado National Renewable Energy Laboratory's (NREL) September 2023 National Pyrheliometer Comparison (NPC) to the World Radiation Reference Maintained at the Physikalisch-Meteorologisches Observatorium Davos / World Radiation Center. The NREL cavity reference group attended the International Pyrheliometer Comparison held in Davos during September and October of 2021, and is therefore traceable to the World Radiation Reference.

The sensitivity factor and its associated uncertainty (95%) are as follows:

Manufacturer	Serial Number	$\mu\text{V}/(\text{W}/\text{m}^2)$	U95
Kipp and Zonen WMO number 39017	CH1-960133	10.637	$\pm 0.532\%$

Application

$$I = (\text{mV output})/S \pm \text{sqrt}(2)*U95\%$$

Where: I = the irradiance measured by the pyrheliometer

(mV output) = microvolt output of the pyrheliometer

S = calibration coefficient of the pyrheliometer

U95% = the 95 % confidence level of a field measurement.

Supporting information, plots, a list of past calibration values, and a brief description of the calibration process is presented below.

## **CALIBRATION LOCATION**

NASA Langley Hampton VA.

Latitude = 37.1038 deg., Longitude = -76.3872 deg., Elevation = 6 meters.

## **CALIBRATING PERSON(S)**

Fred Denn, Bryan Fabbri

## **TRACEABILITY**

The reference standard was Eppley Laboratories Inc., absolute cavity radiometer AHF31041, with its associated, Campbell 1000x based, data acquisition system. The cavity calibration is traceable first to the cavity working group at the National Renewable Energy Laboratory (NREL) in Golden Colorado, And through the NREL group to the World Radiation Reference (WRR), located at the Physikalisch-Meteorologisches Observatorium, in Davos Switzerland. The NREL working group attended the 2021 International Pyrheliometer Intercomparison (IPC). Cavity AHF31041 participated National Pyrheliometer Comparisons (NPC)s at NREL in September and October 2022 and 2023.

## **HARDWARE CONFIGURATION**

The pyrheliometer was mounted on a sun tracker and aligned with the sun.

## **DATA DAYS**

Data were collected during the intervals indicated in below. Test pyrheliometer data are calibrated against cavity pyrheliometer data taken each common second during runs of approximately twenty-five minutes starting on the hour and half hour.

### Date Interval

2026-04-21 13:00:00 through 21:30:00

2026-04-23 13:30:00 through 15:00:00

2026-04-27 13:30:00 through 21:00:00


2026-05-04 14:00:00 through 17:30:00

2026-05-05 13:30:00 through 21:00:00


2026-05-08 12:30:00 through 21:30:00

### Pyrheliometer Calibration Plot

- /Users/fdenn/Forsun/SRB/Calibrations/cavity\_second\_based/Cal\_ch1/groups\_ch1\_960133\_2026-04-21.dat
- /Users/fdenn/Forsun/SRB/Calibrations/cavity\_second\_based/Cal\_ch1/groups\_ch1\_960133\_2026-04-23.dat
- ◇ /Users/fdenn/Forsun/SRB/Calibrations/cavity\_second\_based/Cal\_ch1/groups\_ch1\_960133\_2026-04-27.dat
- △ /Users/fdenn/Forsun/SRB/Calibrations/cavity\_second\_based/Cal\_ch1/groups\_ch1\_960133\_2026-05-04.dat
- ▵ /Users/fdenn/Forsun/SRB/Calibrations/cavity\_second\_based/Cal\_ch1/groups\_ch1\_960133\_2026-05-05.dat
- ▽ /Users/fdenn/Forsun/SRB/Calibrations/cavity\_second\_based/Cal\_ch1/groups\_ch1\_960133\_2026-05-08.dat

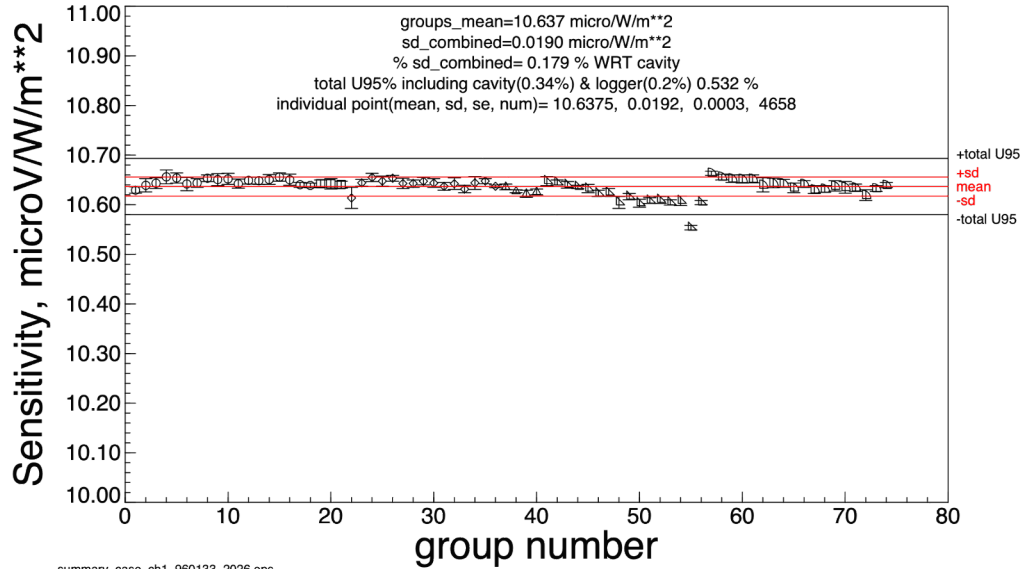

Calibration coefficients for several days. Each symbol represents a cavity run which is approximately 25 minutes. These data are combined to get a final calibration coefficient for the entire, multi-day, calibration session.

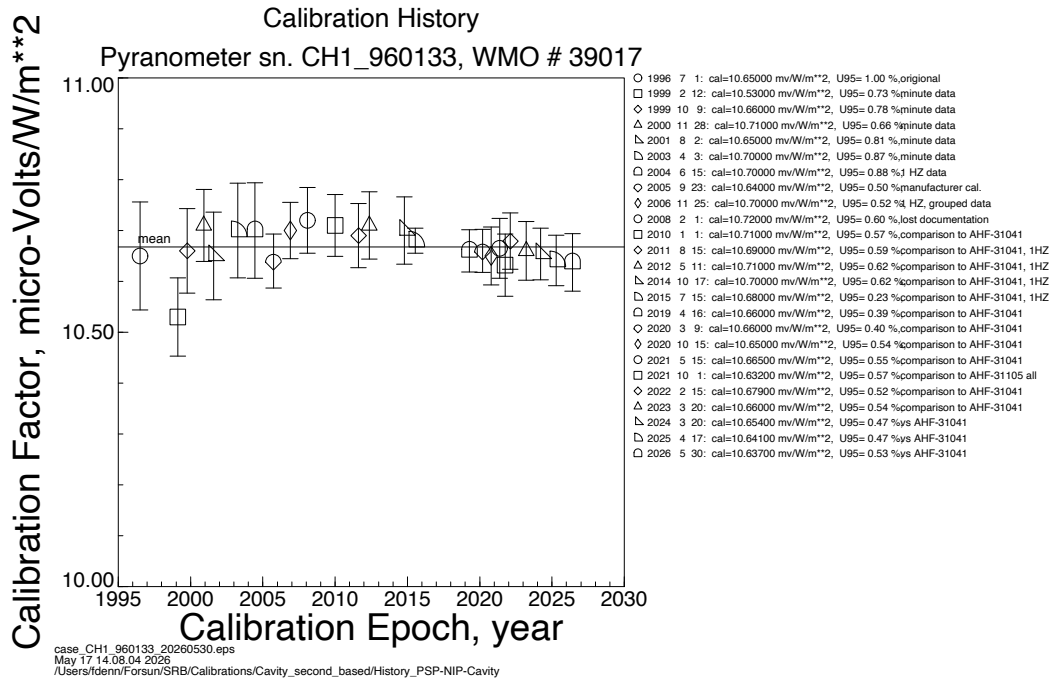

Calibration history for pyrheliometer CH1-960133. The solid horizontal line represents the mean value. The symbols and their error bars represent the mean and U95 of each calibration event. The column on the right presents numerical values for each calibration event and a brief description of the calibration method used.

## CALIBRATION HISTORIES

Pyrheliometer: Kipp and Zonen CH1-960133.

date	S ( $\mu\text{V}/(\text{W}/\text{m}^2)$ )	U95 (%)	Note
2026 May 30	10.637	0.532	1HZ, ref. AHF-31041
2025 Apr 17	10.641	0.47	1HZ, ref. AHF-31041
2024 Mar 20	10.654	0.48	1HZ, ref. AHF-31041
2023 Mar 20	10.660	0.54	1HZ, ref. AHF-31041
2022 Mar 01	10.679	0.52	1HZ, ref. AHF-31041
2020 Oct 15	10.65	0.54	1HZ, ref. AHF-31041
2020 Mar 09	10.658	0.50	1HZ, ref. AHF-31041
2019 Apr 16	10.66	0.50	1HZ, ref. AHF-31041
2015 Jul 15	10.68	0.23	1HZ, ref. AHF-31041
2014 Nov 17	10.70	0.62	1HZ, ref. AHF-31041
2012 May 11	10.71	0.62	1HZ, ref. AHF-31041
2011 Sep 01	10.69	0.59	1HZ, ref. AHF-31041
2010 Jan 01	10.71	0.57	comparison to AHF-31041
2008 Feb 01	10.72	0.60	lost document
2006 Nov 25	10.70	0.58	(1 HZ grouped data)
2006 May 10			Setup error, no useable data.
2005 Sep 23	10.64	0.50	(manufacturer calibration)
2005 Jun 15			Failed, sent in for repairs.
2004 Jul 15	10.70	0.88	(1 HZ data)
2003 Apr 02	10.70	0.87	(minute data)
2001 Aug 02	10.65	0.81	(minute data)
2000 Nov 28	10.71	0.66	(minute data)
1999 Oct 09	10.66	0.78	(minute data)
1999 Feb 12	10.53	0.73	(minute data)
1996 Jun 30	10.65	0.50	(manufacturer calibration)

## **A Very Brief Description of the Calibration Process.**

- 1) Pyranometers are to be mounted horizontally, while pyrhemometers are to be mounted on the tracker pointing at the sun.
- 2) Deploy the Cavity Radiometer, select the 4 second data collection parameter file. Start the cavity calibration process.
- 3) Modify the field radiometer program, so that a file of second data is produced in addition to the minute resolution data file.
- 4) Prepare the tracker hardware to operate in manual shade/unshade mode. Either in manual mode or with the automatic pneumatic cylinder.
- 5) Start the cavity system, first calibrating the cavity, then collecting data for about 20 minutes before doing a recalibration. Repeat the calibration/measure process for the entire calibration period.
- 6) Collect pyranometer data in the unshaded configuration for about 5.0 minutes, and in the shaded configuration for about 5.0 minutes.
- 7) Continue this process while sky conditions permit while cavity irradiance is greater than 700 Watts/meter\*\*2.
- 8) Transfer the cavity and pyranometer data to the data processing computer.
- 9) Remove unstable (greater than 1 w/m\*\*2 variation over 3 seconds) in the cavity data file. This depends on which cavity control system is used.
- 10) Run a splitter program on the field radiometer file to generate a separate file for the shaded and unshaded periods for each instrument.
- 11) Run a plotting program on each data file so the data can be reviewed for: cloud events; bad shading; errors in the splitting routine; etc. Remove bad data records.
- 12) Run calibration programs to determine the calibration coefficient for each instrument.
- 13) Combine several days of calibration data to get a final calibration coefficient.
- 14) Produce a calibration document, such as this one, for each instrument. To be considered valid, a calibration must be documented and traceable to recognized standards, in this case the World Radiation Reference (WRR) in Davos Switzerland.